

# GHD Services Inc.

2055 Niagara Falls Blvd. #3  
Niagara Falls, New York 14304

## Vantage Specialty Chemicals

Gurnee, IL

Project #11197003

Sampling Date: 06.27.19

### Analytical Report (0719-001)

### *EPA Method TO-15 Analysis*

Ethylene oxide



### **Enthalpy Analytical, LLC**

Phone: (919) 850 - 4392 / Fax: (919) 850 - 9012 / [www.enthalpy.com](http://www.enthalpy.com)  
800-1 Capitola Drive Durham, NC 27713-4385

I certify that to the best of my knowledge all analytical data presented in this report:

- Have been checked for completeness
- Are accurate, error-free, and legible
- Have been conducted in accordance with approved protocol, and that all deviations and analytical problems are summarized in the appropriate narrative(s)

This analytical report was prepared in Portable Document Format (.PDF) and contains ??? pages.

Report Issued: xx/xx/xxxx



# Results

Sample Name : AIR-11197003-06272019-041  
 Sample Info : 0719-001; 500mL load; Can#1625  
 Data File : X1902370.D  
 Dilution : 1  
 Pressurization Factor : 1.826  
 Acquisition Date : 2019-07-12 00:33:28  
 Instrument Method : TO15\_RMP\_EO.M  
 Matrix : AIR

Target Compound	Concentration (PPBV)	RL (PPBV)	MDL (PPBV)	Concentration (ug/m3)	RL (ug/m3)	MDL (ug/m3)	Flag *
Ethylene oxide	0.126	0.0183	0.0183	0.227	0.0329	0.0329	m

Internal Standards	Response	Retention Time (min)	Concentration (PPBV)	Flag *
Bromochloromethane (IS)	1,141,191	11.94	5.00	PASS

(ND) = Not Detected  
 \* (J) = Below Calibration Range, (E) = Above Calibration Range, (m) = Manual Integration  
 IS Acceptance Criteria: RT +/- 20 sec, Response +/- 40%

Sample Name : AIR-11197003-06272019-042  
 Sample Info : 0719-001; 500mL load; Can#1623  
 Data File : X1902371.D  
 Dilution : 1  
 Pressurization Factor : 1.729  
 Acquisition Date : 2019-07-12 01:29:38  
 Instrument Method : TO15\_RMP\_EO.M  
 Matrix : AIR

Target Compound	Concentration (PPBV)	RL (PPBV)	MDL (PPBV)	Concentration (ug/m3)	RL (ug/m3)	MDL (ug/m3)	Flag *
Ethylene oxide	ND	0.0173	0.0173	ND	0.0312	0.0312	

Internal Standards	Response	Retention Time (min)	Concentration (PPBV)	Flag *
Bromochloromethane (IS)	1,159,768	11.94	5.00	PASS

(ND) = Not Detected

\* (J) = Below Calibration Range, (E) = Above Calibration Range, (m) = Manual Integration

IS Acceptance Criteria: RT +/- 20 sec, Response +/- 40%

Sample Name : AIR-11197003-06272019-043  
 Sample Info : 0719-001; 500mL load; Can#0736  
 Data File : X1902373.D  
 Dilution : 1  
 Pressurization Factor : 1.744  
 Acquisition Date : 2019-07-12 03:22:11  
 Instrument Method : TO15\_RMP\_EO.M  
 Matrix : AIR

Target Compound	Concentration (PPBV)	RL (PPBV)	MDL (PPBV)	Concentration (ug/m3)	RL (ug/m3)	MDL (ug/m3)	Flag *
Ethylene oxide	0.145	0.0174	0.0174	0.261	0.0314	0.0314	m

Internal Standards	Response	Retention Time (min)	Concentration (PPBV)	Flag *
Bromochloromethane (IS)	1,170,959	11.94	5.00	PASS

(ND) = Not Detected  
 \* (J) = Below Calibration Range, (E) = Above Calibration Range, (m) = Manual Integration  
 IS Acceptance Criteria: RT +/- 20 sec, Response +/- 40%

Sample Name : AIR-11197003-06272019-044  
 Sample Info : 0719-001; 500mL load; Can#0751  
 Data File : X1902374.D  
 Dilution : 1  
 Pressurization Factor : 1.721  
 Acquisition Date : 2019-07-12 04:18:29  
 Instrument Method : TO15\_RMP\_EO.M  
 Matrix : AIR

Target Compound	Concentration (PPBV)	RL (PPBV)	MDL (PPBV)	Concentration (ug/m3)	RL (ug/m3)	MDL (ug/m3)	Flag *
Ethylene oxide	0.255	0.0172	0.0172	0.459	0.0310	0.0310	m

Internal Standards	Response	Retention Time (min)	Concentration (PPBV)	Flag *
Bromochloromethane (IS)	1,169,471	11.95	5.00	PASS

(ND) = Not Detected  
 \* (J) = Below Calibration Range, (E) = Above Calibration Range, (m) = Manual Integration  
 IS Acceptance Criteria: RT +/- 20 sec, Response +/- 40%

Sample Name : AIR-11197003-06272019-045  
 Sample Info : 0719-001; 500mL load; Can#24086  
 Data File : X1902375.D  
 Dilution : 1  
 Pressurization Factor : 1.734  
 Acquisition Date : 2019-07-12 05:14:45  
 Instrument Method : TO15\_RMP\_EO.M  
 Matrix : AIR

Target Compound	Concentration (PPBV)	RL (PPBV)	MDL (PPBV)	Concentration (ug/m3)	RL (ug/m3)	MDL (ug/m3)	Flag *
Ethylene oxide	0.0643	0.0173	0.0173	0.116	0.0312	0.0312	m

Internal Standards	Response	Retention Time (min)	Concentration (PPBV)	Flag *
Bromochloromethane (IS)	1,178,236	11.94	5.00	PASS

(ND) = Not Detected  
 \* (J) = Below Calibration Range, (E) = Above Calibration Range, (m) = Manual Integration  
 IS Acceptance Criteria: RT +/- 20 sec, Response +/- 40%

Sample Name : AIR-11197003-06272019-046  
 Sample Info : 0719-001; 500mL load; Can#24091  
 Data File : X1902376.D  
 Dilution : 1  
 Pressurization Factor : 1.793  
 Acquisition Date : 2019-07-12 06:11:03  
 Instrument Method : TO15\_RMP\_EO.M  
 Matrix : AIR

Target Compound	Concentration (PPBV)	RL (PPBV)	MDL (PPBV)	Concentration (ug/m3)	RL (ug/m3)	MDL (ug/m3)	Flag *
Ethylene oxide	0.0552	0.0179	0.0179	0.0995	0.0323	0.0323	m

Internal Standards	Response	Retention Time (min)	Concentration (PPBV)	Flag *
Bromochloromethane (IS)	1,181,316	11.94	5.00	PASS

(ND) = Not Detected  
 \* (J) = Below Calibration Range, (E) = Above Calibration Range, (m) = Manual Integration  
 IS Acceptance Criteria: RT +/- 20 sec, Response +/- 40%

# Lab QC

Sample Name : AIR-11197003-06272019-042 LD  
 Sample Info : 0719-001; 500mL load; Can#1623  
 Data File : X1902372.D  
 Dilution : 1  
 Pressurization Factor : 1.729  
 Acquisition Date : 2019-07-12 02:25:50  
 Instrument Method : TO15\_RMP\_EO.M  
 Matrix : AIR

Target Compound	Concentration (PPBV)	RL (PPBV)	MDL (PPBV)	Concentration (ug/m3)	RL (ug/m3)	MDL (ug/m3)	% Diff	Flag *
Ethylene oxide	ND	0.0173	0.0173	ND	0.0312	0.0312	NA	

Internal Standards	Response	Retention Time (min)	Concentration (PPBV)	Flag *
Bromochloromethane (IS)	1,161,442	11.94	5.00	PASS

(ND) = Not Detected

\* (J) = Below Calibration Range, (E) = Above Calibration Range, (m) = Manual Integration

IS Acceptance Criteria: RT +/- 20 sec, Response +/- 40%

Sample Name : Humid Blank  
 Sample Info : 500mL load; Can#0702  
 Data File : X1902369.D  
 Dilution : 1  
 Pressurization Factor : 1.000  
 Acquisition Date : 2019-07-11 23:43:42  
 Instrument Method : TO15\_RMP\_EO.M  
 Matrix : AIR

Target Compound	Concentration (PPBV)	RL (PPBV)	MDL (PPBV)	Concentration (ug/m3)	RL (ug/m3)	MDL (ug/m3)	Flag *
Ethylene oxide	ND	0.0100	0.0100	ND	0.0180	0.0180	

Internal Standards	Response	Retention Time (min)	Concentration (PPBV)	Flag *
Bromochloromethane (IS)	1,152,752	11.94	5.00	PASS

(ND) = Not Detected  
 \* (J) = Below Calibration Range, (E) = Above Calibration Range, (m) = Manual Integration  
 IS Acceptance Criteria: RT +/- 20 sec, Response +/- 40%

Sample Name : 1ppbv EO LCS  
Sample Info : 25mL load; Can #0741; GCMSPrepPg0767  
Data File : X1902366.D  
Dilution : 1  
Pressurization Factor : 1.000  
Acquisition Date : 2019-07-11 21:09:57  
Instrument Method : TO15\_RMP\_EO.M  
Matrix : AIR

Target Compound	Response	Concentration (PPBV)	Tag Value (PPBV)	% Recovery	Flag
Ethylene oxide	83,207	0.955	1.01	94.7	PASS

Sample Name : 1ppbv EO LCS  
 Sample Info : 25mL load; Can #0741; GCMSPrepPg0767  
 Data File : X1902366.D  
 Dilution : 1  
 Pressurization Factor : 1.000  
 Acquisition Date : 2019-07-11 21:09:57  
 Instrument Method : TO15\_RMP\_EO.M  
 Matrix : AIR

Target Compound	Concentration (PPBV)	RL (PPBV)	MDL (PPBV)	Concentration (ug/m3)	RL (ug/m3)	MDL (ug/m3)	Flag *
Ethylene oxide	0.955	0.0100	0.0100	1.72	0.0180	0.0180	

Internal Standards	Response	Retention Time (min)	Concentration (PPBV)	Flag *
Bromochloromethane (IS)	1,159,419	11.94	5.00	PASS

(ND) = Not Detected  
 \* (J) = Below Calibration Range, (E) = Above Calibration Range, (m) = Manual Integration  
 IS Acceptance Criteria: RT +/- 20 sec, Response +/- 40%

Sample Name : 0.1ppbv EO Stability Std  
Sample Info : 25mL load; Can #0714; GCMSPrepPg0754  
Data File : X1902368.D  
Dilution : 1  
Pressurization Factor : 1.000  
Acquisition Date : 2019-07-11 22:47:38  
Instrument Method : TO15\_RMP\_EO.M  
Matrix : AIR

Target Compound	Response	Concentration (PPBV)	Tag Value (PPBV)	% Recovery	Flag
Ethylene oxide	10,220	0.120	0.101	118.9	PASS

Sample Name : 0.1ppbv EO Stability Std  
 Sample Info : 25mL load; Can #0714; GCMSPrepPg0754  
 Data File : X1902368.D  
 Dilution : 1  
 Pressurization Factor : 1.000  
 Acquisition Date : 2019-07-11 22:47:38  
 Instrument Method : TO15\_RMP\_EO.M  
 Matrix : AIR

Target Compound	Concentration (PPBV)	RL (PPBV)	MDL (PPBV)	Concentration (ug/m3)	RL (ug/m3)	MDL (ug/m3)	Flag *
Ethylene oxide	0.120	0.0100	0.0100	0.220	0.0183	0.0183	m

Internal Standards	Response	Retention Time (min)	Concentration (PPBV)	Flag *
Bromochloromethane (IS)	1,133,870	11.94	5.00	PASS

(ND) = Not Detected

\* (J) = Below Calibration Range, (E) = Above Calibration Range, (m) = Manual Integration

IS Acceptance Criteria: RT +/- 20 sec, Response +/- 40%

**Canister and Controller Data Sheet****Enthalpy Analytical, LLC**

Client Name: GHD Services, Inc.

Client #: 11197003

Enthalpy Job #: 0719-001

**Canister Data**

Canister ID	Sample ID	Canister Pressure Pre-Sample (mmHg)	Canister Pressure Post-Sample (mmHg)	Canister Pressure Final (mmHg)	Canister Pressurization Factor
1625	0519-259#3	-763	-11	610	1.826
1623	0519-259#3	-763	-8	542	1.729
0736	0519-259#3	-763	-15	541	1.744
0751	0519-259#3	-763	-8	536	1.721
24086	0519-259#3	-763	-21	523	1.734
24091	0519-259#3	-763	-10	587	1.793

Date Prepared: 6/11/19Date Received: 7/1/19

Prepared By: WRC

Received By: DSM

# Narrative Summary

## Enthalpy Analytical Narrative Summary

<b>Company</b>	GHD Services, Inc.
<b>Analyst</b>	TDD
<b>Parameters</b>	EPA Method TO-15 SIM

<b>Client #</b>	11197003
<b>Job #</b>	0719-001
<b># Samples</b>	6 (6L) Canisters

<b>Custody</b>	<p>David Myers received the samples on 7/1/19 after being relinquished by GHD Services, Inc. The samples were received at ambient temperature and in good condition.</p> <p>Prior to, during, and after analysis, the samples were kept under lock with access only to authorized personnel by Enthalpy Analytical, LLC.</p>
<b>Analysis</b>	<p>The samples were analyzed for ethylene oxide using selective ion monitoring (SIM) and analytical procedures from EPA Method TO-15, <i>Determination of Volatile Organic Compounds (VOCs) in Air Collected in Specially-Prepared Canisters and Analyzed by Gas Chromatography/Mass Spectrometry (GC/MS)</i>.</p> <p>Upon receipt, the canister pressures were measured and recorded. The canisters were then pressurized with UHP nitrogen and a dilution ratio was calculated for each canister. Refer to the Canister and Controller Data Sheet in the Lab QC section of this PDF report.</p> <p>The Agilent Technologies Model 6890N, Gas Chromatograph "Xavier" (S/N US10721018) was equipped with a 5975C VL Mass Selective Detector (S/N US71215962) and a Restek Rtx-624 Sil MS, 60 m x 0.32 mm x 1.8 µm capillary column (S/N 1555499) for these analyses. All samples and standards were introduced directly to the analyzer using an Entech 7200 Preconcentrator.</p>
<b>Calibration</b>	<p>The BFB tune analyses associated with the initial and continuing calibrations met method acceptance criteria. The initial calibration (<i>X070919A-EO</i>) that was used to quantitate the samples met the 30% RSD criteria. The initial calibration verification met the 30% recovery criteria. The closing continuing calibration met the 30% response factor difference criteria. Summary calibration data has been included in this report, however full calibration data is available upon request.</p>
<b>Chromatographic Conditions</b>	<p>A copy of the acquisition method (<i>TO15_Rmp_EO.M</i>) is available upon request.</p>



## Enthalpy Analytical Narrative Summary (continued)

### QC Notes

All internal standard retention time and response criteria were met for these analyses.

The laboratory humid blank associated with this analysis did not contain ethylene oxide at a concentration greater than the MDL value.

The laboratory duplicate (LD) analyzed with this batch of samples met the 25% difference acceptance criteria.

The Laboratory Control Sample (LCS) analyzed along with these samples met the  $\pm 30\%$  recovery criteria.

The samples were analyzed within the 30-day holding time required by the method.

### Reporting Notes

These analyses met the requirements of the TNI Standard. Any deviations from the requirements of the reference method or TNI Standard have been stated above.

The results presented in this report are representative of the samples as provided to the laboratory.

# General Reporting Notes

The following are general reporting notes that are applicable to all Enthalpy Analytical, LLC data reports, unless specifically noted otherwise.

- Any analysis which refers to the method as “**Type**” represents a planned deviation from the reference method. For instance a Hydrogen Sulfide assay from a Tedlar bag would be labeled as “EPA Method 16-Type” because Tedlar bags are not mentioned as one of the collection options in EPA Method 16.
- The acronym **MDL** represents the Minimum Detection Limit. Below this value the laboratory cannot determine the presence of the analyte of interest reliably.
- The acronym **LOQ** represents the Limit of Quantification. Below this value the laboratory cannot quantitate the analyte of interest within the criteria of the method.
- The acronym **ND** following a value indicates a non-detect or analytical result below the MDL.
- The letter **J** in the Qualifier or Flag column in the results indicates that the value is between the MDL and the LOQ. The laboratory can positively identify the analyte of interest as present, but the value should be considered an estimate.
- The letter **E** in the Qualifier or Flag column indicates an analytical result exceeding 100% of the highest calibration point. The associated value should be considered as an estimate.
- Sample results are presented ‘as measured’ for single injection methodologies, or an average value if multiple injections are made. If all injections are below the MDL, the sample is considered non-detect and the ND value is presented. If one, but not all, are below the MDL, the MDL value is used for any injections that are below the MDL. For example, if the MDL is 0.500 and LOQ is 1.00, and the instrument measures 0.355, 0.620, and 0.442 - the result reported is the average of 0.500, 0.620, and 0.500 - - - i.e. 0.540 with a J flag.
- When a spike recovery (Bag Spike, Collocated Spike Train, or liquid matrix spike) is being calculated, the native (unspiked) sample result is used in the calculations, as long as the value is above the MDL. If a sample is ND, then 0 is used as the native amount (not the MDL value).
- The acronym **DF** represents Dilution Factor. This number represents dilution of the sample during the preparation and/or analysis process. The analytical result taken from a laboratory instrument is multiplied by the DF to determine the final undiluted sample results.
- The addition of **MS** to the Sample ID represents a Matrix Spike. An aliquot of an actual sample is spiked with a known amount of analyte so that a percent recovery value can be determined. The MS analysis indicates what effect the sample matrix may have on the target analyte, i.e. whether or not anything in the sample matrix interferes with the analysis of the analyte(s).

# General Reporting Notes

(continued)

- The addition of **MSD** to the Sample ID represents a Matrix Spike Duplicate. Prepared in the same manner as a MS, the use of duplicate matrix spikes allows further confirmation of laboratory quality by showing the consistency of results gained by performing the same steps multiple times.
- The addition of **LD** to the Sample ID represents a Laboratory Duplicate. The analyst prepares an additional aliquot of sample for testing and the results of the duplicate analysis are compared to the initial result. The result should have a difference value of within 10% of the initial result (if the results of the original analysis are greater than the LOQ).
- The addition of **AD** to the Sample ID represents an Alternate Dilution. The analyst prepares an additional aliquot at a different dilution factor (usually double the initial factor). This analysis helps confirm that no additional compound is present and coeluting or sharing absorbance with the analyte of interest, as they would have a different response/absorbance than the analyte of interest.
- The Sample ID **LCS** represents a Laboratory Control Sample. Clean matrix, similar to the client sample matrix, prepared and analyzed by the laboratory using the same reagents, spiking standards and procedures used for the client samples. The LCS is used to assess the control of the laboratory's analytical system. Whenever spikes are prepared for our client projects, two spikes are retained as LCSs. The LCSs are labeled with the associated project number and kept in-house at the appropriate temperature conditions. When the project samples are received for analysis, the LCSs are analyzed to confirm that the analyte could be recovered from the media, separate from the samples which were used on the project and which may have been affected by source matrix, sample collection, and/or sample transport.
- **Significant Figures:** Where the reported value is much greater than unity (1.00) in the units expressed, the number is rounded to a whole number of units, rather than to 3 significant figures. For example, a value of 10,456.45 ug catch is rounded to 10,456 ug. There are five significant digits displayed, but no confidence should be placed on more than two significant digits. In the case of small numbers, generally 3 significant figures are presented, but still only 2 should be used with confidence. Many neat materials are only certified to 3 digits, and as the mathematically correct final result is always 1 digit less than all its pre-cursors - 2 significant figures are what are most defensible.
- **Manual Integration:** The data systems used for processing will flag manually integrated peaks with an "M". There are several reasons a peak may be manually integrated. These reasons will be identified by the following two letter designations on sample chromatograms, if provided in the report. The peak was *not integrated* by the software "NI", the peak was *integrated incorrectly* by the software "II" or the *wrong peak* was integrated by the software "WP". These codes will accompany the analyst's manual integration stamp placed next to the compound name on the chromatogram.

# Sample Custody



# Chain of Custody Record

**Special Handling:**

- Standard Turn Around Time
- Rush Turn Around Time -- Date Needed \_\_\_\_\_
- All TATs Subject to Approval by Enthalpy Analytical
- All Bag/Can Samples Disposed of 1 Month from Receipt.
- All Other Samples Disposed of 4 Months from Receipt.

Sample(s) Collected by: Youna Yang  
 Client Name: GHD  
 Project Manager: Matt Lazaric

Project Number: 11197003  
 Site Name: Gura Vantage  
 Location: Gurnee, IL

PO#: \_\_\_\_\_  
 Telephone#: 773-380-9933  
 Email: matthew.lazaric@ghd.com

For spiked or duplicate samples: please provide sample volumes for recovery calculations. For Particulates: please provide tare weights and/or condensed water volumes.

Special Instructions:

A=Air 1=H2SO4 2=NaOH W=Water O=Other  
 X=XAD C=Charcoal SG=Silica Gel  
 G=Grab C=Composite Q=Quality Control O=Other

**Sample Containers**      **Analyses:**

Sample ID	Date	Time	Sample Volume	Type	Matrix	# of VOA Vials	# of Glass	# of Plastic	# of Bags	# of Canisters	# of Tubes	# Other	Analyses	Notes	Can ID #
AIR-11197003-6/27/2019-041	6/27/2019	11:20	6L	C	A					1			Ethylene Oxide X	11:01 AM	1625
AIR-11197003-6/27/2019-042	6/27/2019	11:37	6L	C	A					1			X	11:10 AM	1623
AIR-11197003-6/27/2019-043	6/27/2019	11:54	6L	C	A					1			X	11:18 AM	0736
AIR-11197003-6/27/2019-044	6/27/2019	11:50	6L	C	A					1			X	11:18 AM	0751
AIR-11197003-6/27/2019-045	6/27/2019	12:16	6L	C	A					1			X	11:38 AM	24086
AIR-11197003-6/27/2019-046	6/27/2019	12:37	6L	C	A					1			X	11:59 AM	24091


End time  
 6/28/2019  
 Notes:

Relinquished By:	Date:	Received By:	Date:	Time:	Sample Condition Upon Receipt:
	6/28/2019		7-1-19	6:56 AM	<input type="checkbox"/> Iced <input type="checkbox"/> Ambient <input type="checkbox"/> °C _____ <input type="checkbox"/> Iced <input type="checkbox"/> Ambient <input type="checkbox"/> °C _____ <input type="checkbox"/> Iced <input type="checkbox"/> Ambient <input type="checkbox"/> °C _____

Good Condition Ambient Temp DSM 07-01-19



# Sample Chromatograms

Sample Name : AIR-11197003-06272019-041  
Sample Info : 0719-001; 500mL load; Can#1625  
Data File : X1902370.D  
Dilution : 1  
Pressurization Factor : 1.826  
Acquisition Date : 2019-07-12 00:33:28  
Instrument Method : TO15\_RMP\_EO.M  
Matrix : AIR

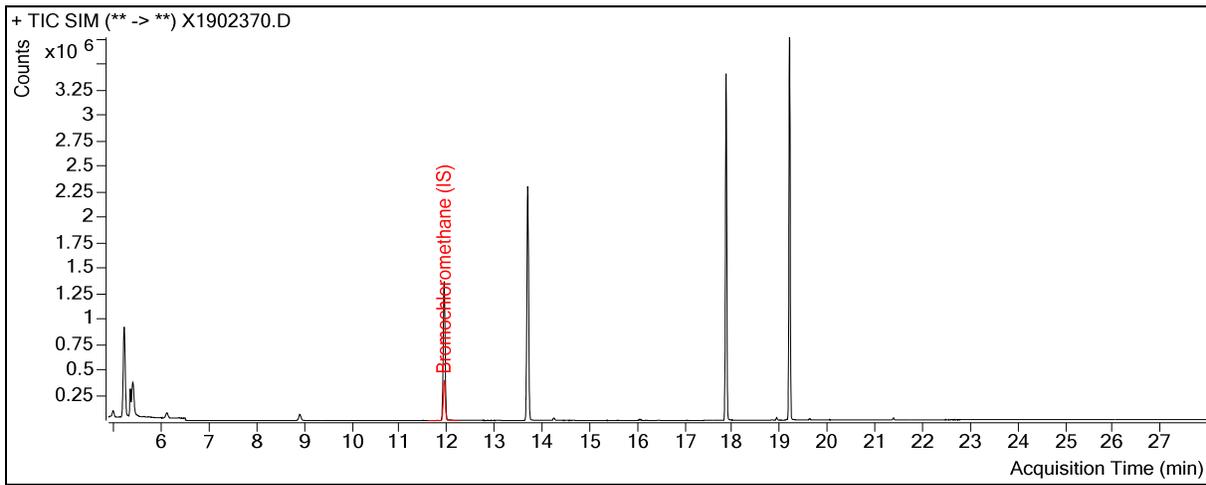


Sample Name : AIR-11197003-06272019-041  
Sample Info : 0719-001; 500mL load; Can#1625  
Data File : X1902370.D  
Dilution : 1  
Pressurization Factor : 1.826  
Acquisition Date : 2019-07-12 00:33:28  
Instrument Method : TO15\_RMP\_EO.M  
Matrix : AIR


Ethylene oxide

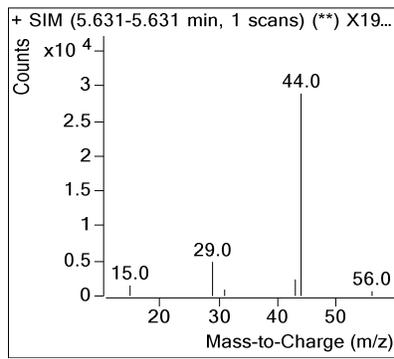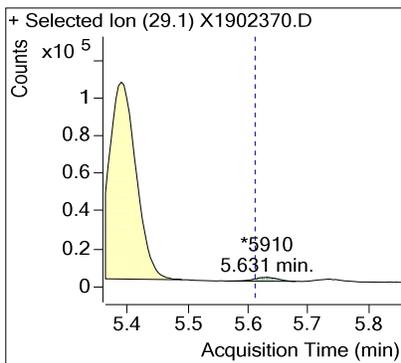


Sample Name : AIR-11197003-06272019-042  
Sample Info : 0719-001; 500mL load; Can#1623  
Data File : X1902371.D  
Dilution : 1  
Pressurization Factor : 1.729  
Acquisition Date : 2019-07-12 01:29:38  
Instrument Method : TO15\_RMP\_EO.M  
Matrix : AIR

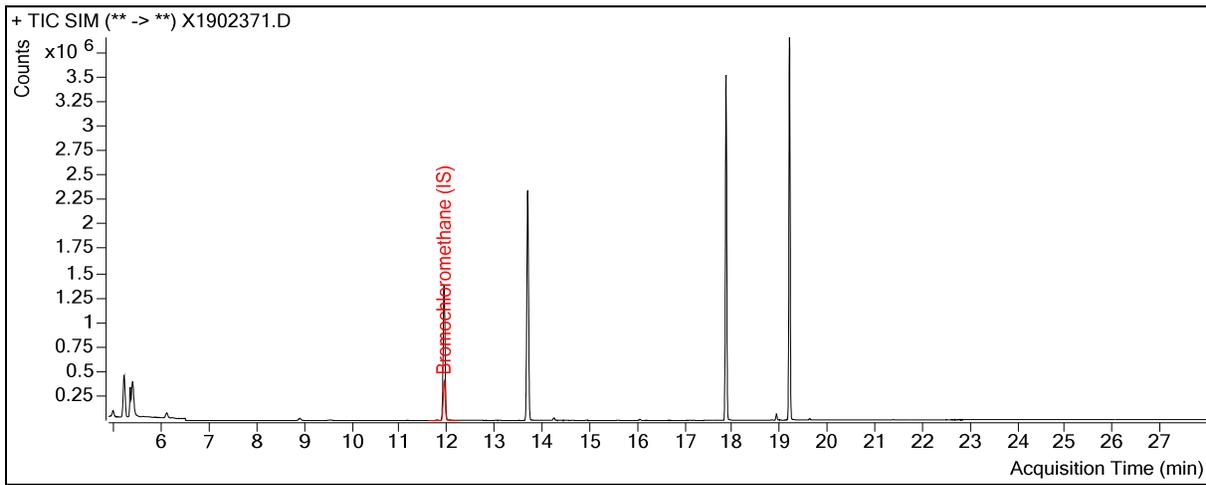

Sample Name : AIR-11197003-06272019-042 LD  
Sample Info : 0719-001; 500mL load; Can#1623  
Data File : X1902372.D  
Dilution : 1  
Pressurization Factor : 1.729  
Acquisition Date : 2019-07-12 02:25:50  
Instrument Method : TO15\_RMP\_EO.M  
Matrix : AIR


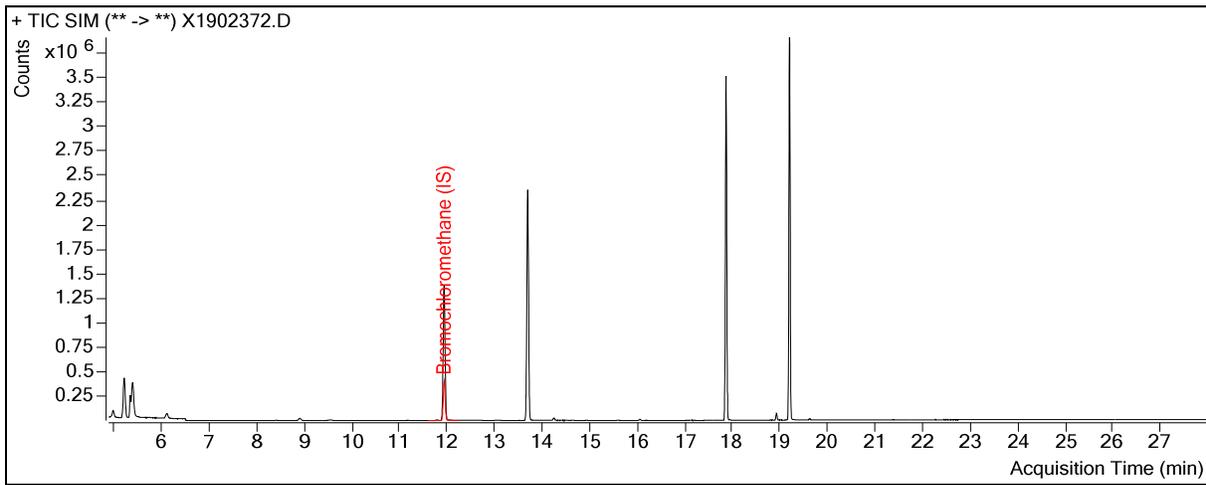


Sample Name : AIR-11197003-06272019-043  
Sample Info : 0719-001; 500mL load; Can#0736  
Data File : X1902373.D  
Dilution : 1  
Pressurization Factor : 1.744  
Acquisition Date : 2019-07-12 03:22:11  
Instrument Method : TO15\_RMP\_EO.M  
Matrix : AIR

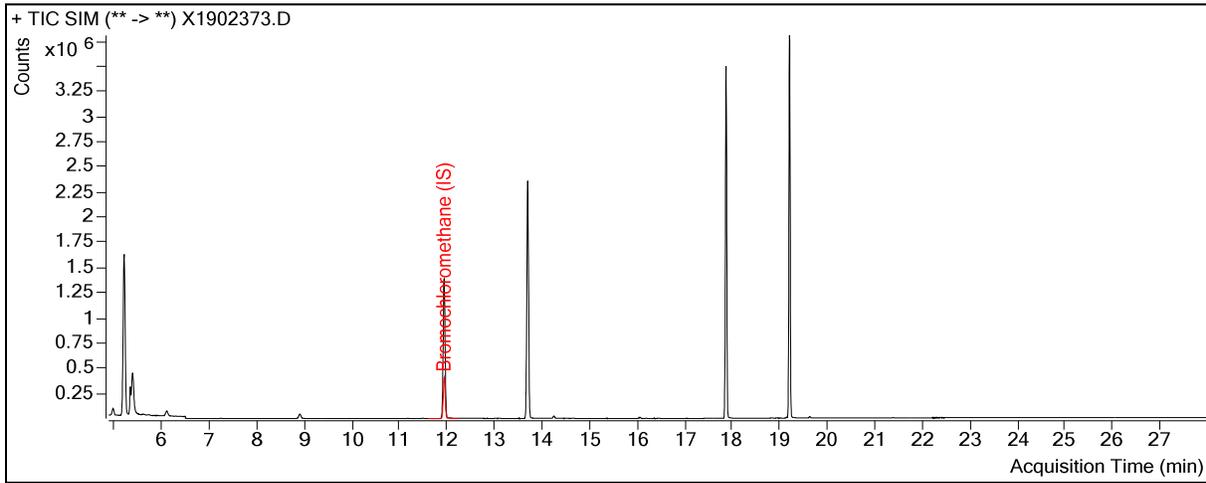


Sample Name : AIR-11197003-06272019-043  
Sample Info : 0719-001; 500mL load; Can#0736  
Data File : X1902373.D  
Dilution : 1  
Pressurization Factor : 1.744  
Acquisition Date : 2019-07-12 03:22:11  
Instrument Method : TO15\_RMP\_EO.M  
Matrix : AIR

Ethylene oxide

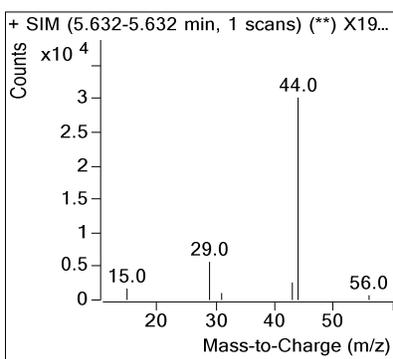
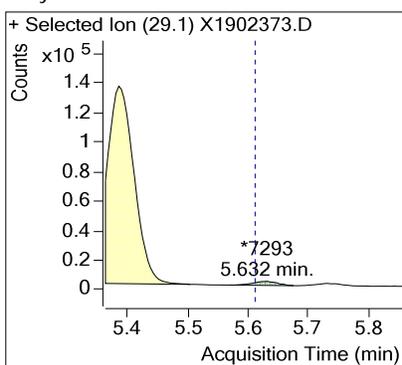


Sample Name : AIR-11197003-06272019-044  
Sample Info : 0719-001; 500mL load; Can#0751  
Data File : X1902374.D  
Dilution : 1  
Pressurization Factor : 1.721  
Acquisition Date : 2019-07-12 04:18:29  
Instrument Method : TO15\_RMP\_EO.M  
Matrix : AIR

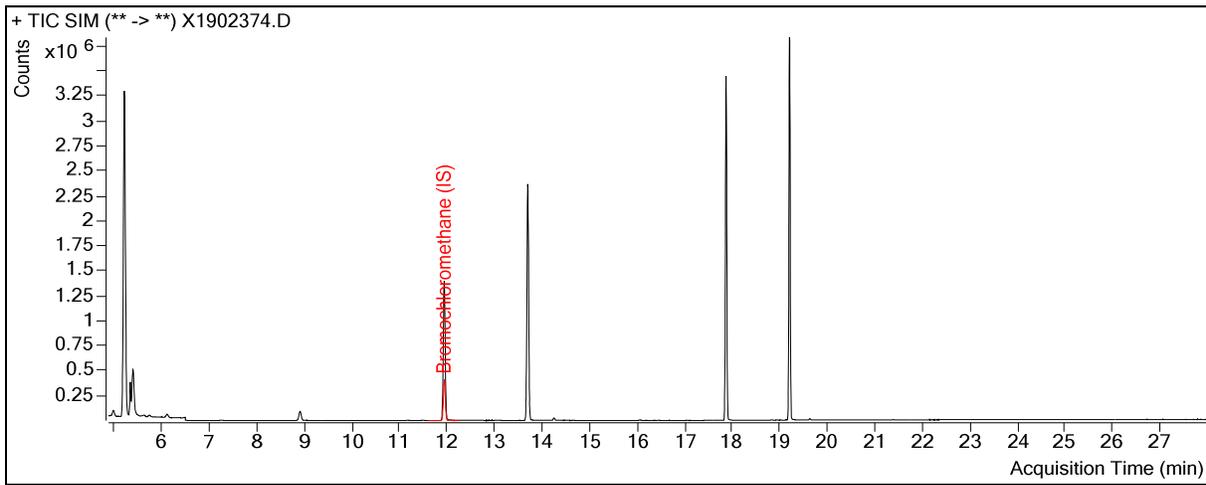


Sample Name : AIR-11197003-06272019-044  
Sample Info : 0719-001; 500mL load; Can#0751  
Data File : X1902374.D  
Dilution : 1  
Pressurization Factor : 1.721  
Acquisition Date : 2019-07-12 04:18:29  
Instrument Method : TO15\_RMP\_EO.M  
Matrix : AIR

Ethylene oxide

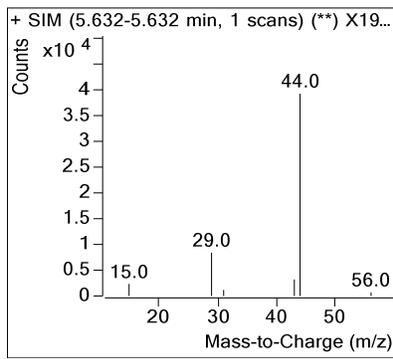
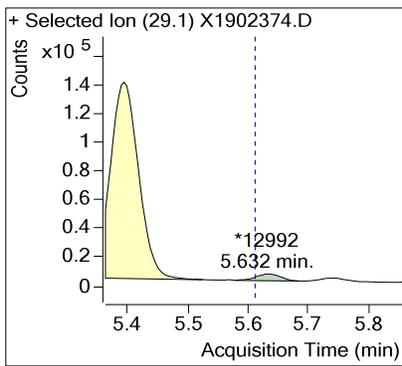


Sample Name : AIR-11197003-06272019-045  
Sample Info : 0719-001; 500mL load; Can#24086  
Data File : X1902375.D  
Dilution : 1  
Pressurization Factor : 1.734  
Acquisition Date : 2019-07-12 05:14:45  
Instrument Method : TO15\_RMP\_EO.M  
Matrix : AIR

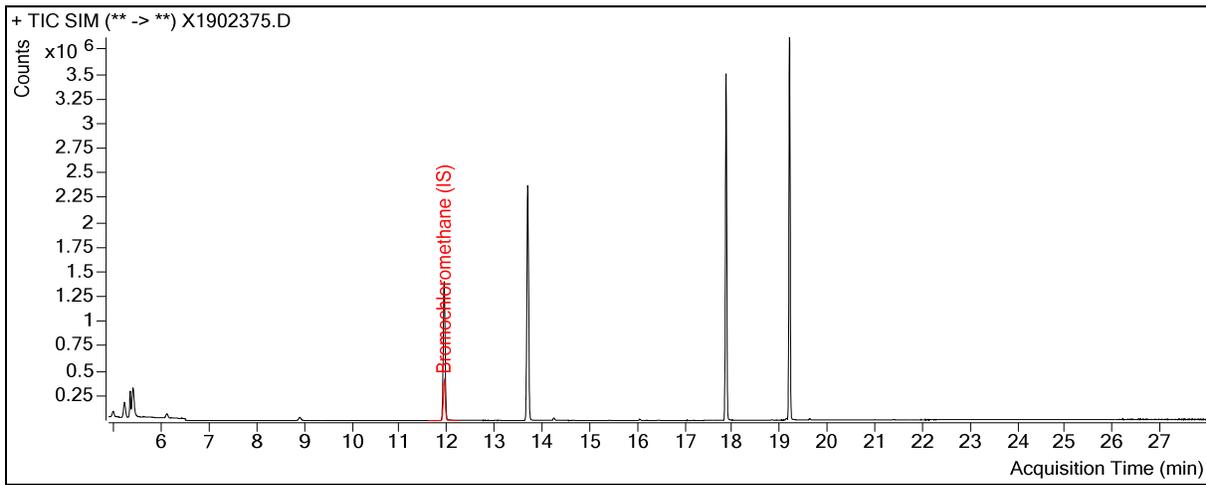


Sample Name : AIR-11197003-06272019-045  
Sample Info : 0719-001; 500mL load; Can#24086  
Data File : X1902375.D  
Dilution : 1  
Pressurization Factor : 1.734  
Acquisition Date : 2019-07-12 05:14:45  
Instrument Method : TO15\_RMP\_EO.M  
Matrix : AIR

Ethylene oxide

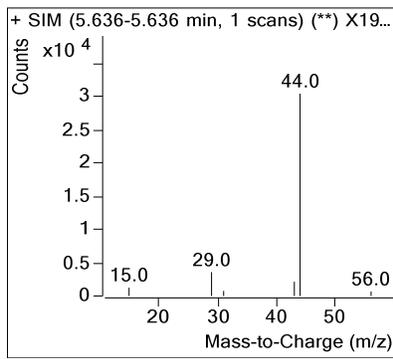
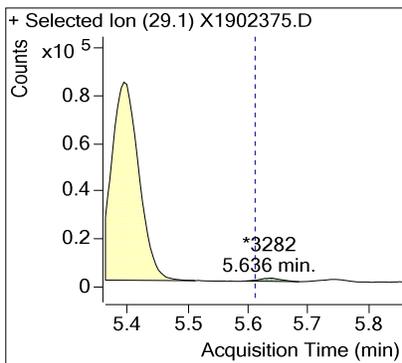


Sample Name : AIR-11197003-06272019-046  
Sample Info : 0719-001; 500mL load; Can#24091  
Data File : X1902376.D  
Dilution : 1  
Pressurization Factor : 1.793  
Acquisition Date : 2019-07-12 06:11:03  
Instrument Method : TO15\_RMP\_EO.M  
Matrix : AIR

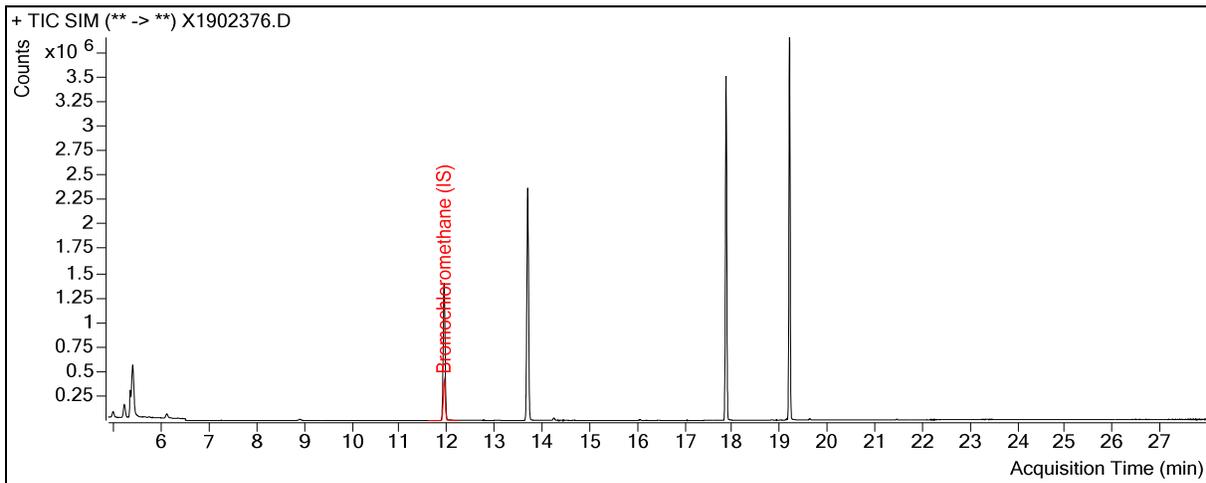


Sample Name : AIR-11197003-06272019-046  
Sample Info : 0719-001; 500mL load; Can#24091  
Data File : X1902376.D  
Dilution : 1  
Pressurization Factor : 1.793  
Acquisition Date : 2019-07-12 06:11:03  
Instrument Method : TO15\_RMP\_EO.M  
Matrix : AIR


Ethylene oxide

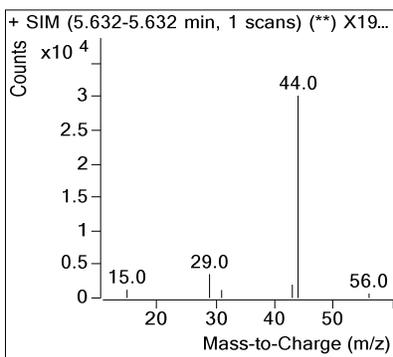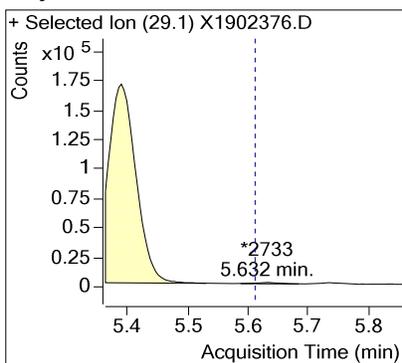


Sample Name : Humid Blank  
Sample Info : 500mL load; Can#0702  
Data File : X1902369.D  
Dilution : 1  
Pressurization Factor : 1.000  
Acquisition Date : 2019-07-11 23:43:42  
Instrument Method : TO15\_RMP\_EO.M  
Matrix : AIR

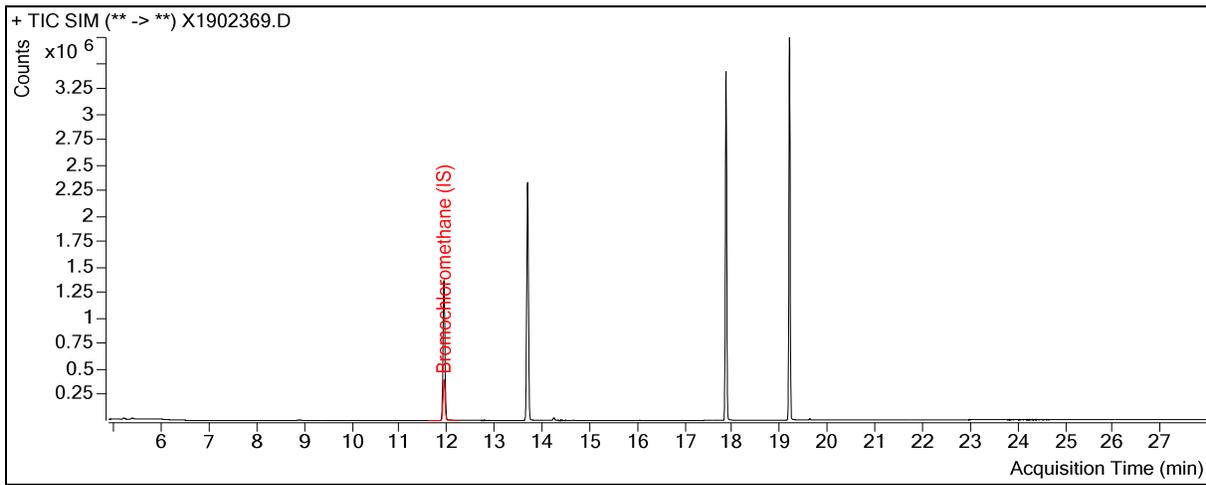

Sample Name : 1ppbv EO LCS  
Sample Info : 25mL load; Can #0741; GCMSPrepPg0767  
Data File : X1902366.D  
Dilution : 1  
Pressurization Factor : 1.000  
Acquisition Date : 2019-07-11 21:09:57  
Instrument Method : TO15\_RMP\_EO.M  
Matrix : AIR


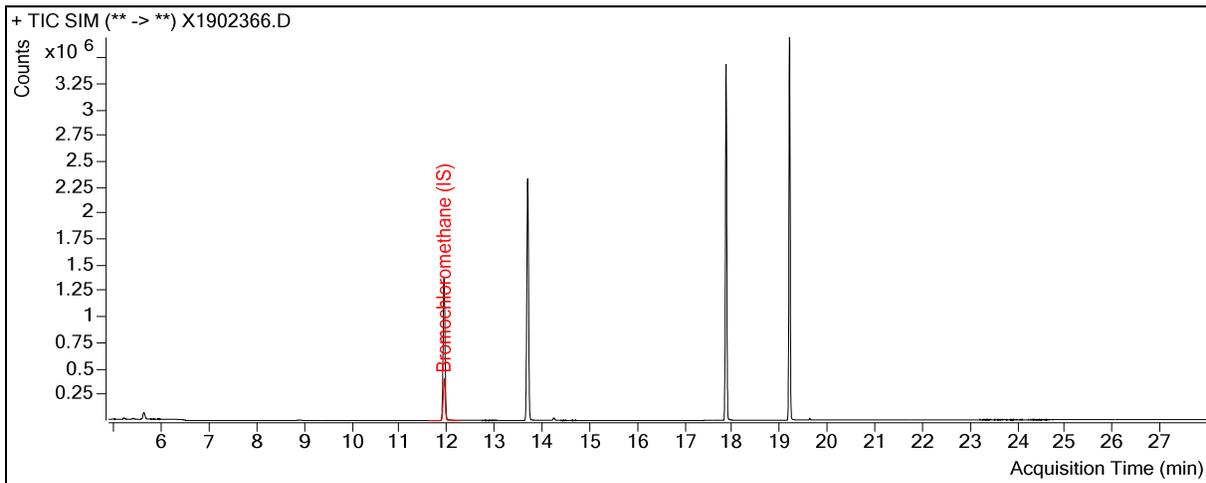


Sample Name : 0.1ppbv EO Stability Std  
Sample Info : 25mL load; Can #0714; GCMSPrepPg0754  
Data File : X1902368.D  
Dilution : 1  
Pressurization Factor : 1.000  
Acquisition Date : 2019-07-11 22:47:38  
Instrument Method : TO15\_RMP\_EO.M  
Matrix : AIR

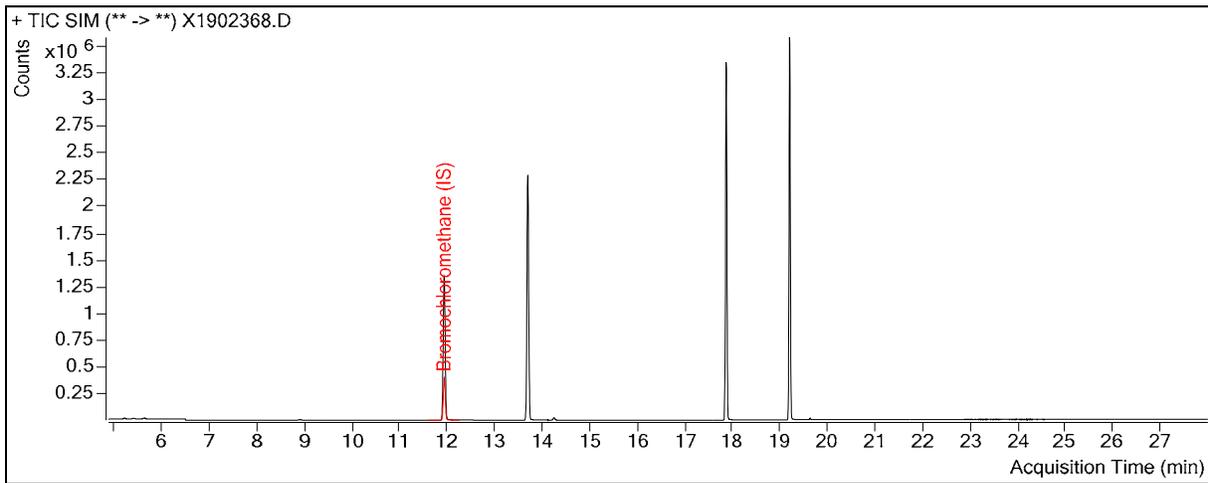

Sample Name : 0.1ppbv EO Stability Std  
Sample Info : 25mL load; Can #0714; GCMSPrepPg0754  
Data File : X1902368.D  
Dilution : 1  
Pressurization Factor : 1.000  
Acquisition Date : 2019-07-11 22:47:38  
Instrument Method : TO15\_RMP\_EO.M  
Matrix : AIR

Ethylene oxide

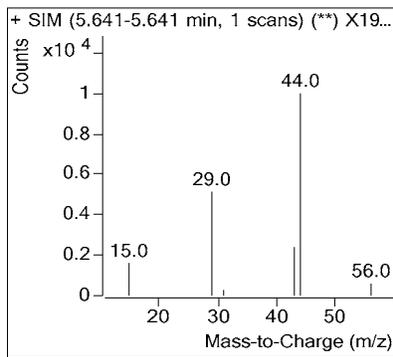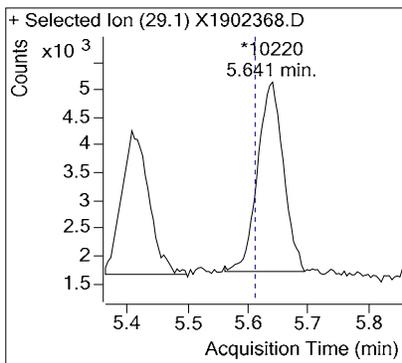

# Calibration Summary Reports

**Calibration Sequence**  
**Method Generation Date**

X070919A-EO Ical.batch.bin  
 7/10/2019

<b>Compound</b>	<b>Type</b>	<b>RT</b>	<b>Average RRT</b>	<b>Average RF</b>	<b>%RSD</b>	<b>Flag</b>
Ethylene oxide	Target	5.61	0.470	0.376	9.67	PASS
Bromochloromethane (IS)	ISTD	11.94	-----	-----	-----	-----

Sample Name : 1ppbv EO ICV  
Sample Info : 25mL load; Can #0741; GCMSPrepPg0767  
Data File : X1902321.D  
Dilution : 1  
Pressurization Factor : 1.000  
Acquisition Date : 2019-07-09 22:18:27  
Instrument Method : TO15\_RMP\_EO.M  
Matrix : AIR

<b>Target Compound</b>	<b>Response</b>	<b>Concentration (PPBV)</b>	<b>Tag Value (PPBV)</b>	<b>% Recovery</b>	<b>Flag</b>
Ethylene oxide	73,432	0.916	1.01	90.8	PASS

Sample Name : 0.5ppbv EO CCV  
Sample Info : 125mL load; Can #2085; GCMSPrepPg0771  
Data File : X1902365.D  
Dilution : N/A  
Pressurization Factor : N/A  
Acquisition Date : 2019-07-11 20:20:46  
Instrument Method : TO15\_RMP\_EO.M  
Matrix : AIR

Target Compound	Response	RF	Average RF	% Difference	Flag
Ethylene oxide	44,528	0.384	0.376	2.3	PASS

Sample Name : 0.5ppbv EO CCV  
Sample Info : 125mL load; Can #2085; GCMSPrepPg0771  
Data File : X1902392.D  
Dilution : N/A  
Pressurization Factor : N/A  
Acquisition Date : 2019-07-12 20:10:50  
Instrument Method : TO15\_RMP\_EO.M  
Matrix : AIR

<b>Target Compound</b>	<b>Response</b>	<b>RF</b>	<b>Average RF</b>	<b>% Difference</b>	<b>Flag</b>
Ethylene oxide	44,281	0.375	0.376	-0.3	PASS

**This Is The Last Page  
Of This Report.**